

MULTIGATE

Vienna™

Anti-Embolism Stockings




Perfect fit every time — the Vienna system makes it easy to fit patients with the correct stockings. With less points of measurement and a simple colour coded system, it's easy to select the right product first time, every time.

Knee

To determine size for knee high stockings:


- 1 Measure **ankle circumference** to determine the size.
- 2 Measure **calf circumference** to ensure the limb fits within the parameters of the determined size.

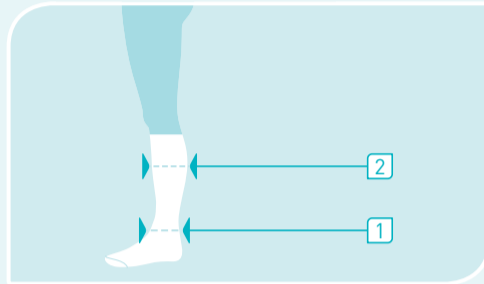


KNEE HIGH STOCKING SIZES

SIZE	CODE	CIRCUMFERENCE (cm)		LEG LENGTH (cm)
		ANKLE	CALF	Heel to back of knee
XS	68-300	19-22	25.5-36	35-39
S	68-301	22-25	33-40	35-39
M	68-311	25-28	38-45	39-44
L	68-321	28-31	43-50	39-44
XL	68-331	31-34	46-53	39-44
XXL	68-341	34-37	49-56	40-45
XXXL	68-351	37-40	53-66	40-45


To apply knee high stockings:

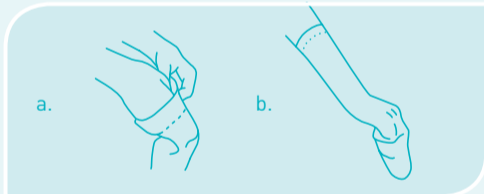

- 1 Insert hand into stocking down to heel pocket.

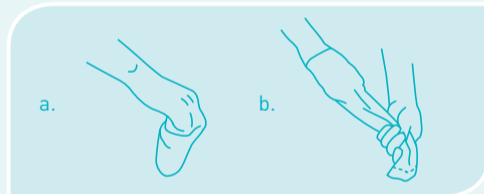

- 2 Grasp heel pocket and turn stocking inside out to heel area.

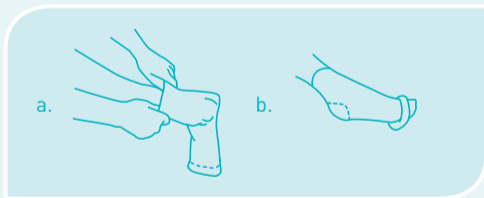

- 3 Carefully pull stocking over foot and heel.




- 4 Pull stocking up to about 2.5-5cm below bottom of knee cap. Smooth excess material out.

- CAUTION**
- Do not turn down top of stocking
 - Do not cover any part of the knee
 - Ensure the use of correct size stocking

Thigh

To determine size for thigh high stockings:


- 1 Measure **ankle circumference** to determine the size.
- 2 Measure **calf circumference** to ensure the limb fits within the parameters of the determined size.
- 3 Measure **thigh circumference** to ensure the limb fits within the parameters of the determined size.

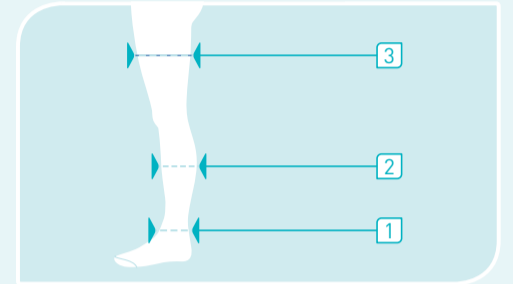


THIGH HIGH STOCKING SIZES

SIZE	CODE	CIRCUMFERENCE (cm)			LEG LENGTH (cm)
		ANKLE	CALF	THIGH	Heel to top of thigh
XS	68-400	19-22	25.5-36	44-56	62-70
S	68-401	22-25	33-40	50-62	62-70
M	68-411	25-28	38-45	56-68	70-80
L	68-421	28-31	43-50	62-74	70-80
XL	68-431	31-34	46-53	68-80	70-80
XXL	68-441	34-37	49-56	74-86	75-83
XXXL	68-451	37-40	53-66	80-92	75-83


To apply thigh high stockings:

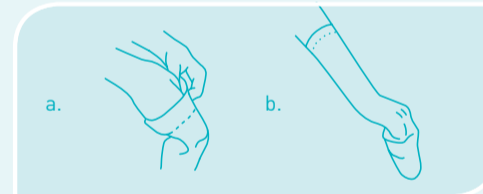


- 1 Insert hand into stocking down to heel pocket.

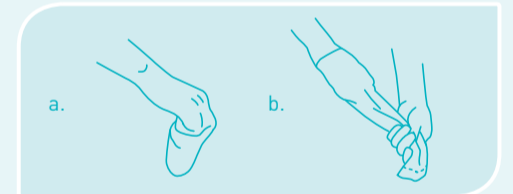

- 2 Grasp heel pocket and turn stocking inside out to heel area.

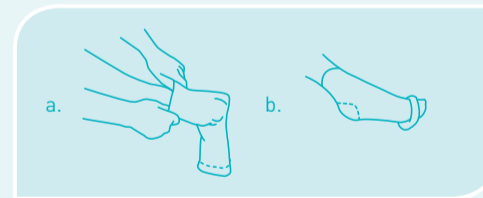

- 3 Carefully pull stocking over foot and heel.

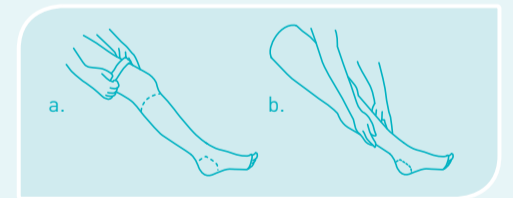

- 4 Pull the remaining stocking up to the top of the thigh. The thigh band sits 1cm below the gluteal furrow. Smooth out the excess material and ensure there are no creases.

- CAUTION**
- Do not turn down top of stocking
 - Ensure the use of correct size stocking

Contraindications

Stockings are not recommended for patients with the following conditions:

- X Any leg condition in which stockings would interfere, such as:
 - a. dermatitis
 - b. vein ligation (immediate postoperative)
 - c. gangrene
 - d. recent skin graft

- X Severe arteriosclerosis or any other ischemic vascular disease
- X Massive oedema of legs or pulmonary oedema from congestive heart failure
- X Extreme deformity of leg.



For more information please contact your Business Development Manager:

(02) 8718 2888 or visit multigate.com.au